



Standard Test Method for Nonmetallic Inclusion Content of Powders Intended for Powder Forging (P/F) Applications¹

This standard is issued under the fixed designation B 796; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers a metallographic method for determining the nonmetallic inclusion level of powders intended for powder forging (P/F) applications.

1.2 The test method covers repress powder forged test specimens in which there has been minimal lateral material flow (<1%). The core region of the powder forged test specimen shall contain no porosity detectable at 100×.

1.3 This test method is not suitable for determining the nonmetallic inclusion level of powder forged test specimens that have been forged such that the core region contains porosity. At the magnification used for this test method residual porosity is hard to distinguish from oxide inclusions. Too much residual porosity makes a meaningful assessment of the inclusion population impossible.

1.4 The test method may be applied to materials that contain manganese sulfide (admixed or prealloyed) provided the near neighbor separation distance is changed from 30 μm to 15 μm.

NOTE 1—The test method may be applied to powder forged parts where there has been a greater amount of material flow provided:

The near neighbor separation distance is changed, or

The inclusion sizes agreed between the parties are adjusted for the amount of material flow.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:

E 3 Practice for Preparation of Metallographic Specimens²

E 768 Guide for Preparing and Evaluating Specimens for Automatic Inclusion Assessment of Steel²

3. Summary of Test Method

3.1 A section representing the core region is cut from the powder forged test specimen and mounted for metallographic grinding and polishing.

3.2 The polished sample is examined microscopically at a magnification of 100× and a note made of inclusions larger than a predetermined size.

3.3 The maximum Feret's diameter is used to determine inclusion size. A Feret's diameter is a caliper diameter as illustrated in Fig. 1.

3.4 The fragmented nature of some inclusions means that their size determination is somewhat complicated. The concept of near neighbor separation is used in determining inclusion size. If an inclusion is within a certain distance of its neighboring particles, it is considered a member of an inclusion cluster or agglomerate. Detected features within 30 μm of one another are considered part of the same inclusion. The concept is illustrated schematically in Fig. 2.

3.5 The nonmetallic inclusion level of the test specimen is reported as the number of inclusions per 100 mm² greater than or equal to the predetermined size.

4. Significance and Use

4.1 The extensive porosity present in pressed and sintered ferrous materials masks the effect of inclusions on mechanical properties. In contrast, the properties of material powder forged to near full density are strongly influenced by the composition, size, size distribution, and location of nonmetallic inclusions.

4.2 The test for nonmetallic inclusions in powder forged steels is useful as the following:

4.2.1 Characteristic to classify or differentiate one grade of powder from another.

4.2.2 Means of quality comparison of powders intended for powder forging, lot to lot.

4.3 Significant variations in nonmetallic inclusion content will occur if:

4.3.1 The powder used to form the test specimen does not meet powder forging quality standards for nonmetallic inclusion content.

¹ This test method is under the jurisdiction of ASTM Committee B09 on Metal Powders and Metal Powder Products and is the direct responsibility of Subcommittee B09.11 on Near Full Density Powder Metallurgy Parts.

Current edition approved April 10, 2002. Published May 2002. Originally published as B – 88. Last previous edition B – 00.

² *Annual Book of ASTM Standards*, Vol 03.01.

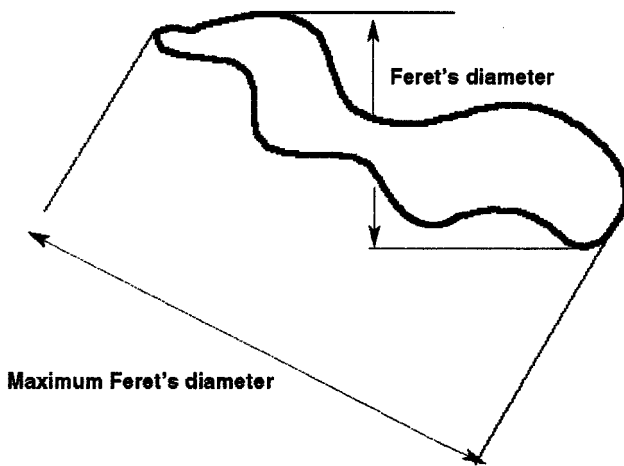


FIG. 1 Schematic illustration of Feret's diameter.

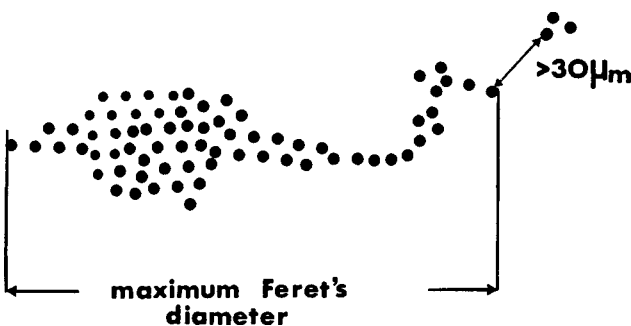


FIG. 2 Schematic illustration of the "near neighbor" concept and maximum Feret's diameter.

4.3.2 Processing of the powder forged test specimen has been carried out under conditions that do not permit oxide reduction or allow oxidation of the test specimen, or both.

5. Apparatus

5.1 Equipment for the metallographic preparation of test specimens.

5.2 A metallographic microscope permitting observation and measurement up to a magnification of $100\times$ using light with a wavelength of 544 nm (green filter), an objective lens with a magnification of from $8\times$ to $12.5\times$, and a numerical aperture between 0.16 and 0.20.

NOTE 2—Defining the light optics used is important because this determines the features that will be resolved, and all detected features are included in the assessment of inclusion size.

6. Sampling

6.1 A metallographic sample shall be removed from the powder forged test specimen, austenitized, and quenched.

6.2 The polished surface of the sample to be examined shall be not less than 350 mm^2 (0.54 in.^2) in area. Multiple sections are permitted in order to obtain the necessary area for measurement.

6.3 The polished surface shall be parallel to the direction of forging, that is, parallel to the direction of travel of the forging punch, and shall represent the core region of the test specimen.

7. Procedure

7.1 *Preparation of Specimens*—In polishing the specimens,

it is highly important that a clean polish be obtained and that the inclusions not be pitted, dragged, or obscured. It is recommended that the procedures described in Practice E 3 and Guide E 768 be followed. Automated grinding and polishing procedures are recommended. Examine specimens in the as-polished condition, free of the effects of any prior etching, if used.

7.2 Measurement of Nonmetallic Inclusion Content:

7.2.1 Survey at least 350 mm^2 (0.54 in.^2) of the surface of the polished specimen at a magnification of $100\times$ using light with a wavelength of 544 nm (green filter), an objective lens with a magnification of from $8\times$ to $12.5\times$, and a numerical aperture between 0.16 and 0.20.

7.2.2 Size detected inclusions on the basis of near neighbor separation. Features within $30\text{ }\mu\text{m}$ of one another are considered to be part of the same inclusion.

7.2.3 For individual features less than $30\text{ }\mu\text{m}$ in size, three such features within $30\text{ }\mu\text{m}$ of one another are required to constitute an inclusion aggregate.

7.2.4 Add an individual feature less than $30\text{ }\mu\text{m}$ in size to an inclusion larger than $30\text{ }\mu\text{m}$, provided both features are within $30\text{ }\mu\text{m}$ of one another. Examples are given in Figs. 3 and 4.

7.2.5 Measure and record the number of inclusion particles according to the principle of near neighbor separation and sized using the maximum Feret's diameter that are as follows:

7.2.5.1 Greater than or equal to $30\text{ }\mu\text{m}$ but less than $100\text{ }\mu\text{m}$ in length,

7.2.5.2 Greater than or equal to $100\text{ }\mu\text{m}$ but less than $150\text{ }\mu\text{m}$ in length, and

7.2.5.3 Greater than or equal to $150\text{ }\mu\text{m}$ in length.

8. Report

8.1 Report the number of nonmetallic inclusions per 100 mm^2 that are as follows:

8.1.1 Greater than or equal to $30\text{ }\mu\text{m}$ but less than $100\text{ }\mu\text{m}$ in length.

8.1.2 Greater than or equal to $100\text{ }\mu\text{m}$ but less than $150\text{ }\mu\text{m}$ in length.

8.1.3 Greater than or equal to $150\text{ }\mu\text{m}$ in length.

8.2 The total area examined.



FIG. 3 Example of a spotty oxide inclusion. The maximum Feret's diameter is indicated.

10. Keywords

10.1 nonmetallic inclusions; powder forged (P/F) steel parts

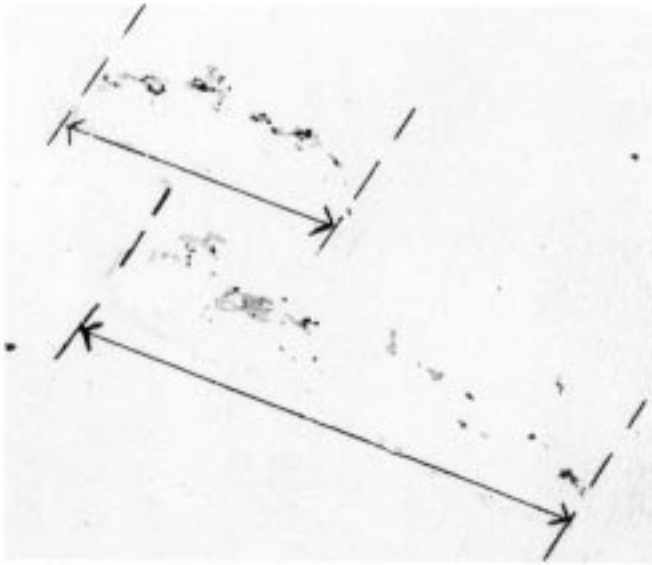


FIG. 4 Example of a discontinuous sulphide inclusion. The maximum Feret's diameter is indicated.

9. Precision and Bias

9.1 The precision and bias that can be expected through the use of this test method is currently under review by Subcommittee B09.11.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).